ALUMINUM FRAME BATH BENCH

MDS89740RW

Weight Capacity: 250 lbs.
Height Range: 14”-20 ¾”
Tool-Free Assembly

THIS PRODUCT CONTAINS DRY NATURAL RUBBER

MEDLINE

Revised 6/16/08

ASSEMBLY INSTRUCTIONS

1. Make sure you have all necessary components for assembling your bath bench.

1 Seat **(A)**
5 Triangular Hand Screws **(B)**
2 Aluminum Mainframes (imprinted A and B) **(C)**
4 Aluminum Extension Legs **(D)**

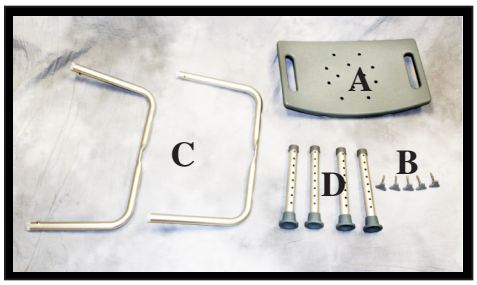

****NOTE:** Upon receipt of package, check ALL parts for shipping damage. If shipping damage is noted, DO NOT USE. Call Medline to report the issue immediately @ 1-800-MEDLINE

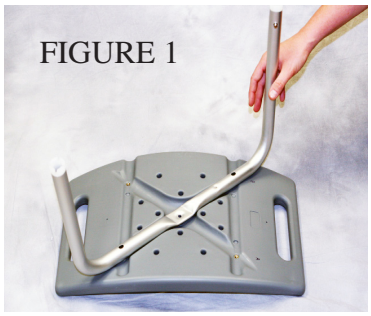

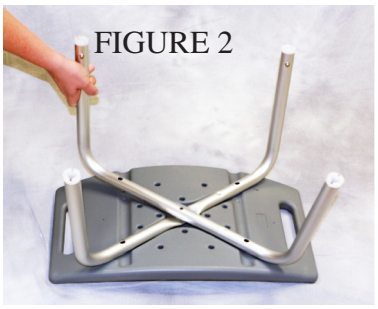

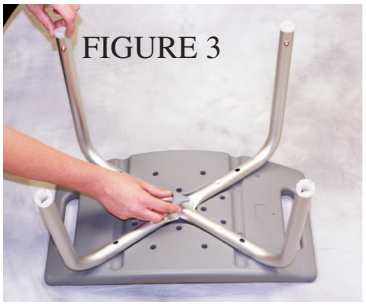

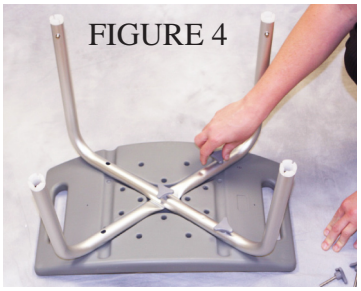

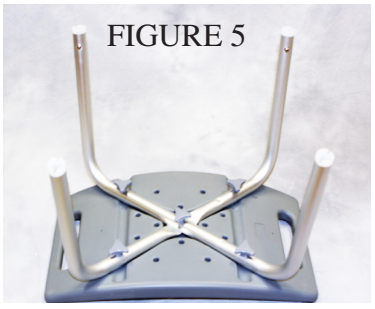

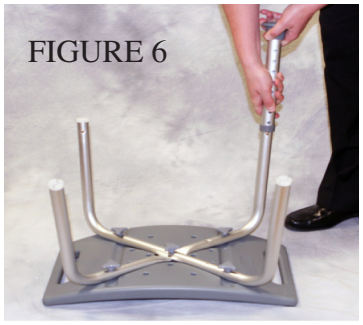

2. Turn seat over to reveal holes for mainframes (See Figure 1). Locate B on bench. Match B from bench with mainframe that is labeled with B. Place B main frame into indentation of bench.

3. Take mainframe A and match it up with A on bench. (See Figure 2)

4. Secure middle hole with 1 triangular hand screw. (See Figure 3) HAND TIGHTEN ONLY!

5. Place remaining triangular hand screws into respected holes of mainframes to secure to bench. (See Figures 4 and 5). HAND TIGHTEN ONLY!!

6. Depress push-buttons on main frame and place aluminum extension legs into mainframe tube and repeat with all legs (See Figure 6). Make sure push-button is fully protruded before using.

** Choose appropriate hole on leg for desired height.

Hole	1	2	3	4	5	6	7	8
Bench Height	14”	15”	16”	17”	18”	19”	19 ¾”	20 ¾”

GENERAL WARNINGS AND INSTALLATION INSTRUCTIONS

PLEASE READ CAREFULLY BEFORE USING YOUR MEDLINE BATH BENCH

To ensure the safe installation, adjustment, and operation of Bath Bench, these instructions MUST be followed:

GENERAL WARNINGS

DO NOT install this product without first reading and understanding this instruction sheet. If you are unable to understand these warnings, cautions, and instructions, contact a healthcare professional or dealer before attempting to install this equipment. Failure to follow instructions may result in serious injury.

- Prior to each use check that all joints and fittings on the bath bench are tight.
- Check that all pushbuttons are fully protruded through holes and are properly engaged.
- Make sure all four legs are adjusted evenly and are free of any obstructions prior to use.
- Check all screws for tightness before **EACH** use.
- **Do not** place bath bench on uneven surfaces.
- **Do not** use if wobbly, unstable or not level.
- **Do not** exceed user weight capacity of 250 lbs.
- **Do not** twist or turn while seated on bath bench, this may cause frame to bend.
- **Do not** stand on bath bench.
- **Do not** use bath bench for any purpose that it is not intended to be used for.
- Check rubber tips for rips, cracks or wear. If these conditions exist, **DO NOT** use the tips and replace **IMMEDIATELY. (Rubber Tips can be ordered--item MDS87755T)**

MEDLINE LIMITED WARRANTY

Your Medline product is warranted to be free of material defects in materials and workmanship for a period of three (3) years from the date of purchase. Non-durable components such as hand grips and push-buttons are warranted for a period of one (1) year from the date of purchase. This express warranty exends only to the original purchaser. This warranty does not extend to damage or failure occuring as a result of owner misusage or negligence, normal wear and tear, or other causes unrelated to the manufacture and design of the product. This express warranty is Medline's sole and exclusive warranty and your sole remedy in the event of default or failure. Medline is not responsible for any consequential or incidental damages or cost arising from the use of the warranted products, or any defect therein or failure thereof.

KEEP YOUR RECEIPT!

Contact us at 1-800-MEDLINE, Monday-Friday 8AM-5PM CST if you encounter and problems or for information regarding repairs or maintenence.

Medline disclaims all other warranties including but not limited to the implied warranties or merchantability and fitness for a particular purpose.